
The KRONNER SIDE-KICK

for holding uterine manipulators

Abbreviated Disassembling Instructions for removing the Ucare setup

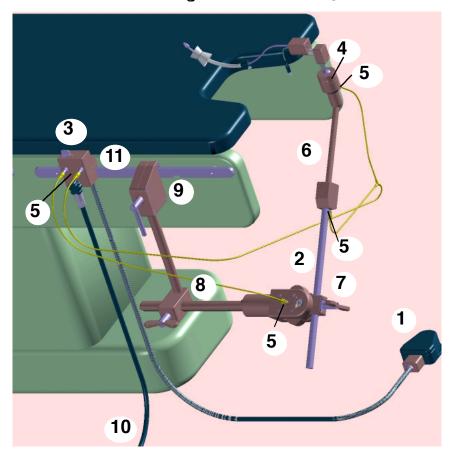

Kronner Medical, 1443 Upper Cleveland Rapids Road, Roseburg, OR 97471 Tel: 541-672-2543

Disassembling SIDEKICK from the Vcare manipulator

- 1. Release the joining screw, step on the foot pedal and detach Sidekick from the manipulator.
- 2. Continue stepping on the foot pedal and lower the arm to the stop. **DO NOT FORCE THE STOP.**
- 3. Shut off the gas switch on the gas supply module.

 This must be done prior to removing the gas lines.
- 4. Disconnect the adapter from the inner rod ball joint.
- 5. Remove the gas lines.
- 6. Remove the inner rod from the outer arm.
- 7. Remove the outer arm from the pivot.

 Perform steps 6 & 7 prior to elevating the dropped table section. Dropped table section not shown.
- 8. Remove the pivot from the rail grip.
- 9. Remove the rail grip from the table rail.
- 10. Detach the gas module supply hose from the wall supply.
- 11. Detach the gas supply module from the table rail.

Remove the manipulator.

